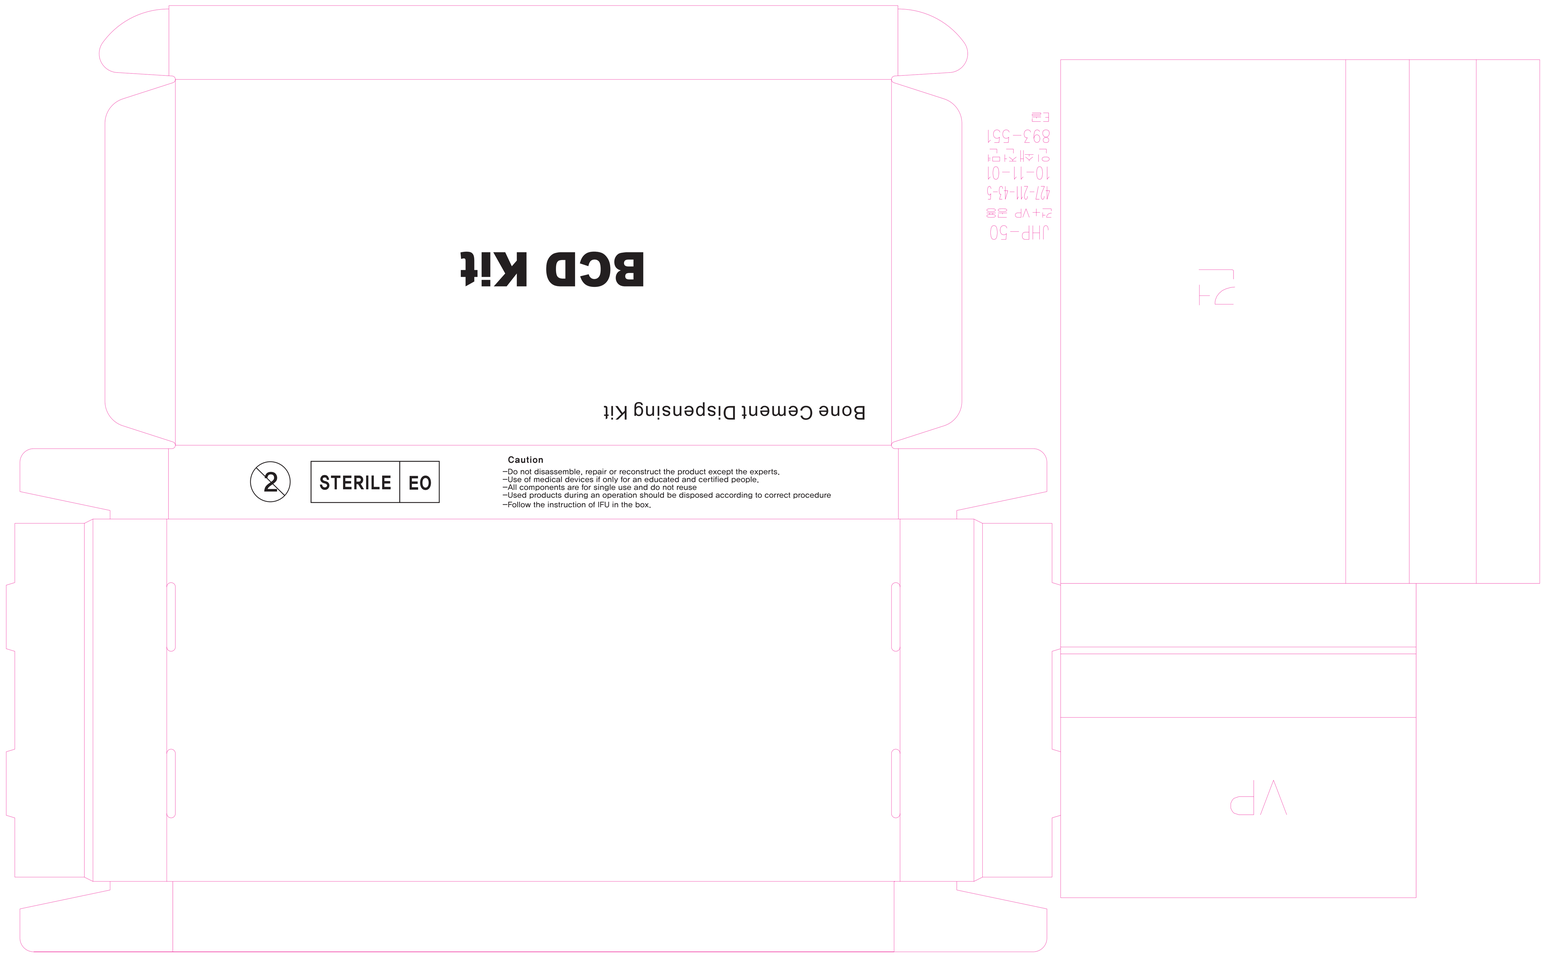
BCD Kit
Bone Cement Dispensing Kit
STERILE EO
Caution
–Do not disassemble, repair or reconstruct the product except the experts.
–Use of medical devices if only for an educated and certified people.
–All components are for single use and do not reuse
–Used products during an operation should be disposed according to correct procedure
–Follow the instruction of IFU in the box.
24
VP